



CALIBRATION CERTIFICATE
 Certificate Number: G00G8RBSMZ-0
 Order Number: 222-586



Customer Houston Forensic Science Center **Location** 500 Jefferson St **Serial Number** 042780009
 Jennifer OCallaghan
 500 Jefferson St
 Houston, TX 77002-7300
Model VWR HIGH PERFORMANCE PIPETTOR 5000 µl
Next Service Jul.2023
Service Plan Onsite: Single Channel PM, 3x5 AR

Inspection Over All Condition: Good

Preventive Maintenance: Piston cleaned and re-greased
Adjustment: No-Adjustment made




As left-Passed Steven Murray 01.Jul.2022

Conditions	Humidity 56.73 % 56.73 %	Air Temperature 20.17 °C 20.17 °C	Z-Factor 1.0029 µl/mg
	Air Pressure 1013.20 hPa 1013.20 hPa	Water Temperature 20.17 °C 20.17 °C	Evaporation 0 mg
Equipment	Balance C132316237Next Cal. (30.Nov.2022)Readability (0.0001 g)		Pipette Tip Customer Supplied
	Climate Monitor BP (QN400005684)Next Cal. (31.Dec.2022) Humidity - 122594359 (122594359)Next Cal. (31.Aug.2022) Temperature - 122594359 (122594359)Next Cal. (31.Aug.2022)		Specification Type Custom

Test Volume (µl)	Weighings				
	1	2	3	4	5
1000 µl	1018.9 mg	1014.8 mg	1010.4 mg	1012.2 mg	1017.0 mg
2500.0 µl	2513.3 mg	2517.2 mg	2512.3 mg	2513.5 mg	2512.3 mg
5000 µl	4988.6 mg	5003.6 mg	5005.2 mg	4999.6 mg	5012.3 mg

Test Volume (µl)	Mean Volume (µl)	Systematic Error				Random Error				Expanded Uncertainty (µl)	Status
		Error (µl)	Limit (+/- µl)	Error (%)	Limit (+/- %)	Error (µl)	Limit (µl)	Error (CV%)	Limit (%)		
		1000	1018	17.60	30	1.760	3	3.46	30		
2500.0	2521.0	21.01	75	0.8404	3	2.03	75	0.08047	3	7.1 µl (k=2)	Passed
5000	5016	16.37	150	0.3273	3	8.74	150	0.1743	3	26 µl (k=2.87)	Passed

As left History

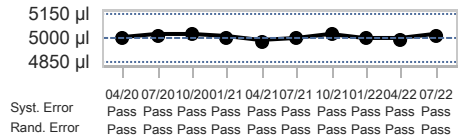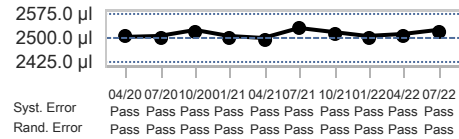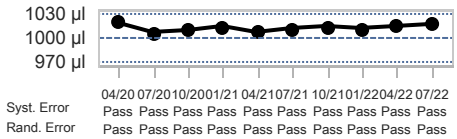

Authorized Signatory, Steven Murray
 01.Jul.2022

METTLER TOLEDO
 ACCREDITED LABORATORY
 7500 Edgewater Drive
 Oakland, CA 94621