



CALIBRATION CERTIFICATE

Certificate Number: H00G83AVHG-0

Order Number: 222-766

RAININ
Pipetting 360°

Customer Houston Forensic Science Center
Jennifer O'Callaghan
500 Jefferson St

Houston, TX 77002-7300

Location 500 Jefferson St

Serial Number PU10413

Model THERMO FINNPIPETTE F2 100-1000 BLUE
Next Service 31.Oct.2024
Service Plan Onsite: Single Channel PM, 3x5 AR

Inspection Over All Condition: Good

Preventive Maintenance: Piston cleaned and re-greased

Adjustment: No-Adjustment made

As left-Passed Steven Murray 30.Oct.2023




Conditions	Humidity	Start End		Air Temperature	Start End	
		49.6 % 49.0 %	19.3 °C 19.2 °C			
	Air Pressure	1012.2 hPa 1012.1 hPa		Water Temperature	19.3 °C 19.2 °C	
Equipment	Balance	C132316237Next Cal. (30.Nov.2023)Readability (0.0001 g)				
	Climate Monitor	Bar. pressure abs. air pressure (2112149)Next Cal. (01.Dec.2023) Humidity (2112149)Next Cal. (01.Dec.2023) Temp (2112149)Next Cal. (01.Dec.2023)				

Z-Factor 1.0028 µl/mg
Evaporation 0 mg
Specification Type Custom
Pipette Tip Customer Supplied

Test Volume (µl)	Weighings				
	1	2	3	4	5
100.0 µl	99.5 mg	98.1 mg	98.2 mg	98.1 mg	97.5 mg
500.0 µl	497.6 mg	498.3 mg	498.7 mg	498.4 mg	498.5 mg
1000 µl	996.4 mg	996.9 mg	997.2 mg	997.7 mg	997.7 mg

Test Volume (µl)	Mean Volume (µl)	Systematic Error				Random Error				Expanded Uncertainty (µl)	Status
		Error (µl)	Limit (+/- µl)	Error (%)	Limit (+/- %)	Error (µl)	Limit (µl)	Error (CV%)	Limit (%)		
		(µl)	(+/- µl)	(%)	(+/- %)	(µl)	(µl)	(CV%)	(%)		
100.0	98.6	-1.44	3.0	-1.445	3.0	0.74	3.0	0.7491	3.0	2.1 µl (k=2.28)	Passed
500.0	499.7	-0.30	15	-0.06095	3.0	0.42	15	0.08395	3.0	1.6 µl (k=2)	Passed
1000	1000.0	-0.03	30	-0.002790	3.0	0.56	30	0.05556	3.0	2.2 µl (k=2)	Passed

As left History

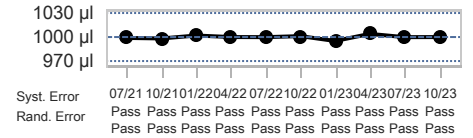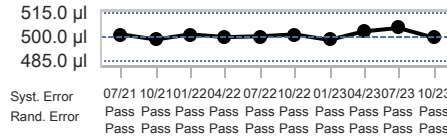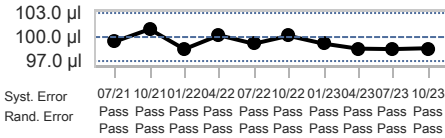

Authorized Signatory, Steven Murray
30.Oct.2023

METTLER TOLEDO
ACCREDITED LABORATORY
7500 Edgewater Drive
Oakland, CA 94621

This calibration covered by this certificate is in accordance with ISO 8655-7:2022 and PS-125. Its measurements are traceable to SI through N.I.S.T. This laboratory has been accredited by A2LA for the requirements of ISO/IEC 17025:2017. The reported expanded uncertainty of measurement (U) is stated as the standard uncertainty of measurement multiplied by the coverage factor k such that the coverage probability corresponds to approximately 95 %. Statement of compliance does not include the measurement of uncertainty. Mettler-Toledo Rainin LLC grants permission to reproduce this document in full only. ©2020 Mettler-Toledo Rainin, LLC