



CALIBRATION CERTIFICATE
 Certificate Number: G00G8RBQN5-0
 Order Number: 222-586



Customer Houston Forensic Science Center **Location** 500 Jefferson St **Serial Number** O495461
 Jennifer OCallaghan
 500 Jefferson St
 Houston, TX 77002-7300
Model EPPENDORF MULTIPETTE M4 1ML COMBITIP
Next Service Jul.2023
Service Plan Onsite: Single Channel PM, 3x5 AR

Inspection Over All Condition: Good

Preventive Maintenance: Cleaned and checked
Adjustment: No-Adjustment made




As left-Passed Steven Murray 01.Jul.2022

Conditions	Humidity 54.16 % 54.16 %	Air Temperature 20.06 °C 20.06 °C	Z-Factor 1.0029 µl/mg
	Air Pressure 1013.20 hPa 1013.20 hPa	Water Temperature 20.06 °C 20.06 °C	Evaporation 0 mg
Equipment	Balance C132316237Next Cal. (30.Nov.2022)Readability (0.0001 g)		Pipette Tip Customer Supplied
	Climate Monitor BP (QN400005684)Next Cal. (31.Dec.2022) Humidity - 122594359 (122594359)Next Cal. (31.Aug.2022) Temperature - 122594359 (122594359)Next Cal. (31.Aug.2022)		Specification Type Custom

Test Volume (µl)	Weighings				
	1	2	3	4	5
20.0 µl	20.7 mg	19.6 mg	20.2 mg	19.5 mg	19.8 mg
100.0 µl	99.8 mg	99.7 mg	99.7 mg	99.7 mg	99.2 mg
200 µl	199.4 mg	199.6 mg	199.2 mg	199.0 mg	200.4 mg

Test Volume (µl)	Mean Volume (µl)	Systematic Error				Random Error				Expanded Uncertainty (µl)	Status
		Error (µl)	Limit (+/- µl)	Error (%)	Limit (+/- %)	Error (µl)	Limit (µl)	Error (CV%)	Limit (%)		
		20.0	20.0	0.02	0.600	0.08942	3.00	0.49	0.600		
100.0	99.91	-0.09	3.00	-0.09110	3.00	0.24	3.00	0.2397	3.00	0.67 µl (k=2.52)	Passed
200	200.1	0.10	6.00	0.04930	3.00	0.54	6.00	0.2708	3.00	1.6 µl (k=2.87)	Passed

As left History

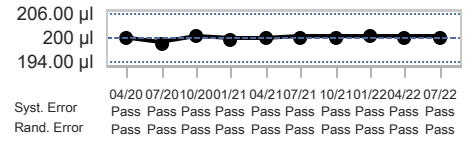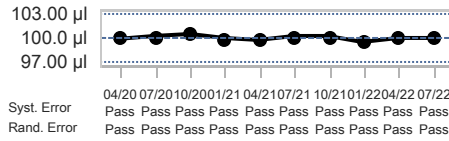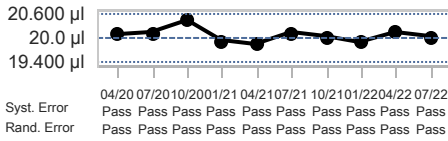

Authorized Signatory, Steven Murray
 01.Jul.2022

METTLER TOLEDO
 ACCREDITED LABORATORY
 7500 Edgewater Drive
 Oakland, CA 94621